




# ARCHER

## 3' or 4' (T8, T5 or T5HO)


### Dimensional Data

Side Profile




Mounting Dimensions

3' Back View

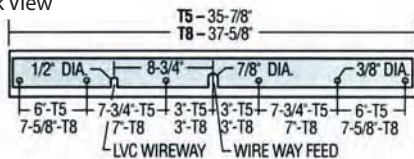

4' Back View

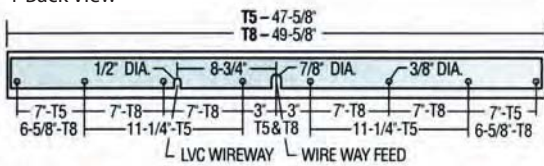

### \*Ordering Notes


For pull chain and pillow switch, specify left or right location as viewed facing the headwall. Optional LED chart light with rocker switch is installed on opposite end of fixture from pull chain location.

Specifications subject to change. Please visit our web site for updated information.

### Specifications

- Construction:** Extruded aluminum housing with stamped aluminum end caps.
- Electrical:** 120 or 277 volt.
- Lamp Shield:** High impact acrylic lens.
- Lamps:** 3 foot nominal: 25w T8, 21w T5 or 39w T5HO lamps (by others).  
4 foot nominal: 32w T8, 28w T5 or 54w T5HO lamps (by others).
- Optional:** (1) 1w LED with rocker switch.
- Seismic:** 3' and 4' units OSHPD pre-approved (OPA-2087-07).
- Finishes:** Polyester powder coated after fabrication with either flat white or designer white antimicrobial finish.
- Listings:** UL and C-UL (1598: Medical and Dental luminaires).
- Warranty:** 5-year limited warranty. Made in the USA by Healthcare Lighting's ISO certified facility in Fairview, PA.

### Photometric Data

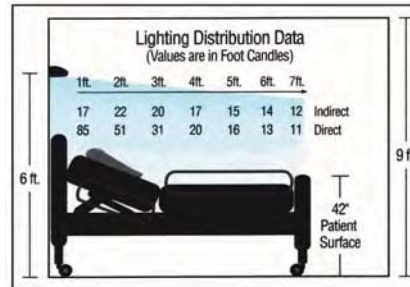

HPW348; data shown with (4) 54w T5HO lamps.

ARCHER

Gundersen Lutheran Hospital  
 Type: **BL1**  
 HPW348-277V-T8EL-11-LC2-XX-FW



### Ordering Information

Example: HPW348-120-T8EL-22-S4L-LED-FW

1	2	3	4	5	6	7
<b>SERIES</b>	<b>VOLTAGE</b>	<b>BALLAST</b>	<b>LAMPING</b>	<b>SWITCHING</b>	<b>OPTIONS</b>	<b>FINISHES</b>
<input type="checkbox"/> HPW336 (36")	<input type="checkbox"/> 120	<input type="checkbox"/> T8EL	<input type="checkbox"/> 11 (1 Up, 1 Down)	<input type="checkbox"/> LC Class 2 UL® rated Low Voltage Controller (LVC)	<input type="checkbox"/> LED 1w white LED chart light*	<input type="checkbox"/> FW Flat white finish
<input type="checkbox"/> HPW348 (48")	<input type="checkbox"/> 277	<input type="checkbox"/> T5EL	<input type="checkbox"/> 21 (2 Up, 1 Down)	<input type="checkbox"/> LC1 LVC with pillow switch controlling down light only	<input type="checkbox"/> BD Bed stop power cut off (Disrupts power to patient bed electrical outlet upon movement of light fixture housing on mounting bracket)	<input type="checkbox"/> AM Designer white antimicrobial finish
		<input type="checkbox"/> T5HO	<input type="checkbox"/> 12 (1 Up, 2 Down)	<input type="checkbox"/> LC2 LVC with pillow switch controlling up and down light sequentially	<input type="checkbox"/> FH Fast-blo fuse	<input type="checkbox"/> CC Custom Color (please provide color # or sample)
			<input type="checkbox"/> 22 (2 Up, 2 Down)	<input type="checkbox"/> S2R On/off pull chain on right (120v only)*	<input type="checkbox"/> SB Slo-blo fuse	
				<input type="checkbox"/> S2L On/off pull chain on left (120v only)*		
				<input type="checkbox"/> S4R 4-pos pull chain on right (120v only)*		
				<input type="checkbox"/> S4L 4-pos pull chain on left (120v only)*		
				<input type="checkbox"/> SX No switch		



# ARCHER

## 3' or 4' (T8, T5 or T5HO)


### Dimensional Data

Side Profile




Mounting Dimensions

3' Back View

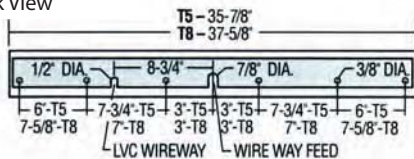

4' Back View

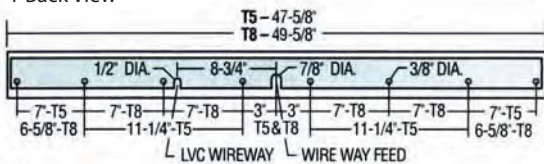

### \*Ordering Notes


For pull chain and pillow switch, specify left or right location as viewed facing the headwall. Optional LED chart light with rocker switch is installed on opposite end of fixture from pull chain location.

Specifications subject to change. Please visit our web site for updated information.

### Specifications

- Construction:** Extruded aluminum housing with stamped aluminum end caps.
- Electrical:** 120 or 277 volt.
- Lamp Shield:** High impact acrylic lens.
- Lamps:** 3 foot nominal: 25w T8, 21w T5 or 39w T5HO lamps (by others).  
4 foot nominal: 32w T8, 28w T5 or 54w T5HO lamps (by others).
- Optional:** (1) 1w LED with rocker switch.
- Seismic:** 3' and 4' units OSHPD pre-approved (OPA-2087-07).
- Finishes:** Polyester powder coated after fabrication with either flat white or designer white antimicrobial finish.
- Listings:** UL and C-UL (1598: Medical and Dental luminaires).
- Warranty:** 5-year limited warranty. Made in the USA by Healthcare Lighting's ISO certified facility in Fairview, PA.

### Photometric Data

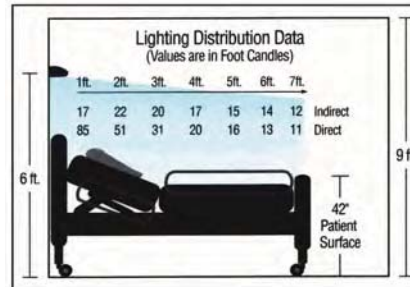

HPW348; data shown with (4) 54w T5HO lamps.

### ARCHER

Gundersen Lutheran Hospital  
 Type: **BL2**  
 HPW336-277V-T8EL-11-LC2-XX-FW



### Ordering Information

Example: HPW348-120-T8EL-22-S4L-LED-FW

1	2	3	4	5	6	7
SERIES	VOLTAGE	BALLAST	LAMPING	SWITCHING	OPTIONS	FINISHES
<input type="checkbox"/> HPW336 (36")	<input type="checkbox"/> 120	<input type="checkbox"/> T8EL	<input type="checkbox"/> 11 (1 Up, 1 Down)	<input type="checkbox"/> LC Class 2 UL® rated Low Voltage Controller (LVC)	<input type="checkbox"/> LED 1w white LED chart light*	<input type="checkbox"/> FW Flat white finish
<input type="checkbox"/> HPW348 (48")	<input type="checkbox"/> 277	<input type="checkbox"/> T5EL	<input type="checkbox"/> 21 (2 Up, 1 Down)	<input type="checkbox"/> LC1 LVC with pillow switch controlling down light only	<input type="checkbox"/> BD Bed stop power cut off (Disrupts power to patient bed electrical outlet upon movement of light fixture housing on mounting bracket)	<input type="checkbox"/> AM Designer white antimicrobial finish
		<input type="checkbox"/> T5HO	<input type="checkbox"/> 12 (1 Up, 2 Down)	<input type="checkbox"/> LC2 LVC with pillow switch controlling up and down light sequentially	<input type="checkbox"/> FH Fast-blo fuse	<input type="checkbox"/> CC Custom Color (please provide color # or sample)
			<input type="checkbox"/> 22 (2 Up, 2 Down)	<input type="checkbox"/> S2R On/off pull chain on right (120v only)*	<input type="checkbox"/> SB Slo-blo fuse	
				<input type="checkbox"/> S2L On/off pull chain on left (120v only)*		
				<input type="checkbox"/> S4R 4-pos pull chain on right (120v only)*		
				<input type="checkbox"/> S4L 4-pos pull chain on left (120v only)*		
				<input type="checkbox"/> SX No switch		